

Safe-T-Vue® 6 • Product No. 7206

Quality Assurance: Safe-T-Vue® 6 Non-Reversible Blood Bag Temperature Indicator Product No. 7206
 PLEASE NOTE: ALL BOX OF 50 INFORMATION AND FOIL LID COPY FOR SAFE-T-VUE® 6 IS PRINTED IN PURPLE.

Lot # **S6 020410**

Expiration Date: February 2012

Non - Chemistry

Mark for "Accepted" and X for "Not Accepted."

Box	Adh. Label	Foil Lid	Close Function	Fill Level
<input checked="" type="checkbox"/> Copy	<input checked="" type="checkbox"/> Copy	<input checked="" type="checkbox"/> Copy	<input checked="" type="checkbox"/> Formed	<input checked="" type="checkbox"/> Acceptable
<input checked="" type="checkbox"/> Tack	<input checked="" type="checkbox"/> Tack	<input checked="" type="checkbox"/> Position	<input checked="" type="checkbox"/> Locked/Stable	<input type="checkbox"/> Underfill
<input checked="" type="checkbox"/> Clean	<input checked="" type="checkbox"/> Color	<input checked="" type="checkbox"/> Clean Peel	Hinge	<input type="checkbox"/> Overfill
<input checked="" type="checkbox"/> Box Damage	Tray	Disk	<input checked="" type="checkbox"/> Elasticity	Color Label
	<input checked="" type="checkbox"/> Edges	<input checked="" type="checkbox"/> Appearance		<input checked="" type="checkbox"/> Color
	<input checked="" type="checkbox"/> Color	<input checked="" type="checkbox"/> Fit		

Test Protocol – Finished Goods Quality Assurance

Test performed on random sampling of finished product per ANSI ASQZ1.4-2003

Data from a "DigiSense" Thermister Electronic Thermometer, using a cold (start temperature 1° to 3° C) bag of simulated blood (10% glycerol-water) with thermometer probe positioned in center of blood bag. Agitation of blood bag necessary for collection of accurate temperature-color change data. Download detailed protocol, from www.williamlabs.com, QCP/0200-5, "Receiving Inspection – Temperature Indicators". [Important: 7206 has a specific incoming inspection protocol.]

Temperature Change and Corresponding Safe-T-Vue® Change

Sample Set 1	DATA	Sample Set 2
1 to 3 °C	Starting Temperatures	1 to 3 °C


OBSERVATIONS

Temperature	Color Change	
4.6 °C	Red Spots - Random	WHITE CENTER
5.4 °C	Red Filling In	WHITE CENTER
6.1 °C	Full Red Color	RED CENTER

Temperature	Color Change	
4.4 °C	Red Spots - Random	WHITE CENTER
5.3 °C	Red Filling In	WHITE CENTER
6.0 °C	Full Red Color	RED CENTER

Temperature accuracy is +/-0.3°C.

Results: Red Spots - Random 4.5 °C; Red Filling in White Center 5.4 °C; Full Red Color at 6.1 °C.

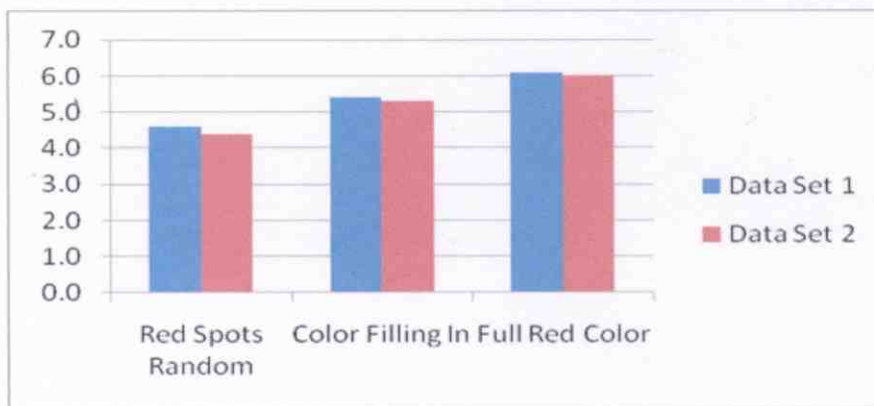

QUALITY ASSURANCE: APPROVED LOT # S6 020410 ; Edward N. Sharpless

QAP/0100-3 REV 03, 09/25/09

Quality Director

February 16, 2010

Date