

Safe-T-Vue® 8 • Product No. 7208

Quality Assurance: Safe-T-Vue® 8 Non-Reversible Blood Bag Temperature Indicator Product No. 7208

PLEASE NOTE: ALL BOX OF 50 INFORMATION AND FOIL LID COPY FOR SAFE-T-VUE® 8 IS PRINTED IN GREEN (PMS 327).

Test performed on Random Sampling of Finished Product Lot # **S8 100110**

Expiration Date: 2012-10

Non - Chemistry

Mark for "accepted" and X for "Not Accepted".

Box	Adh. Label	Foil Lid	Close Function	Fill Level
<input checked="" type="checkbox"/> Copy	<input checked="" type="checkbox"/> Copy	<input checked="" type="checkbox"/> Copy	<input checked="" type="checkbox"/> Formed	<input checked="" type="checkbox"/> Acceptable
<input checked="" type="checkbox"/> Tack	<input checked="" type="checkbox"/> Tack	<input checked="" type="checkbox"/> Position	<input checked="" type="checkbox"/> Locked/Stable	Underfill
<input checked="" type="checkbox"/> Clean	<input checked="" type="checkbox"/> Color	<input checked="" type="checkbox"/> Clean Peel	Hinge	Overfill
<input checked="" type="checkbox"/> Box Damage	Tray	Disk	<input checked="" type="checkbox"/> Elasticity	Color Label
	<input checked="" type="checkbox"/> Edges	<input checked="" type="checkbox"/> Appearance		Color
	<input checked="" type="checkbox"/> Color	<input checked="" type="checkbox"/> Fit		

Test Protocol – Finished Goods Quality Assurance

Test performed on random sampling of finished product per ANSI ASQZ1.4-2003

Performed by using a "DigiSense" Thermister Electronic Thermometer. Using a cold (1° to 4° C) bag of simulated blood (a glycerol-water-red dye solution) with the electric thermometer placed and sealed into the core of the blood bag to permit observation of temperature changes. For detailed protocol request QAP 0300-01 REV 0 Mar 01, 2005 [Incoming inspection of 7208 follows the same protocol for Safe-T-Vue® 10]

Temperature Change and Corresponding Safe-T-Vue® Change

Sample Set 1	DATA	Sample Set 2
1 to 4 °C	Starting Temperatures	1 to 4 °C

OBSERVATIONS


Temperature	Condition	
7.2 °C	Red Spots - Random	WHITE CENTER
7.8 °C	Red Filling In	WHITE CENTER
8.1 °C	Full Red Color	RED CENTER

Temperature	Condition	
7.1 °C	Red Spots - Random	WHITE CENTER
7.7 °C	Red Filling In	WHITE CENTER
8.0 °C	Full Red Color	RED CENTER

Temperature accuracy is +/-0.3°C.

Results of Testing Lot # **S8 100110**; Test Date: October 13, 2010

Red Spots - Random 7.2°C; Red Filling in White Center 7.8 °C; Full Red Color at 8.1° C.

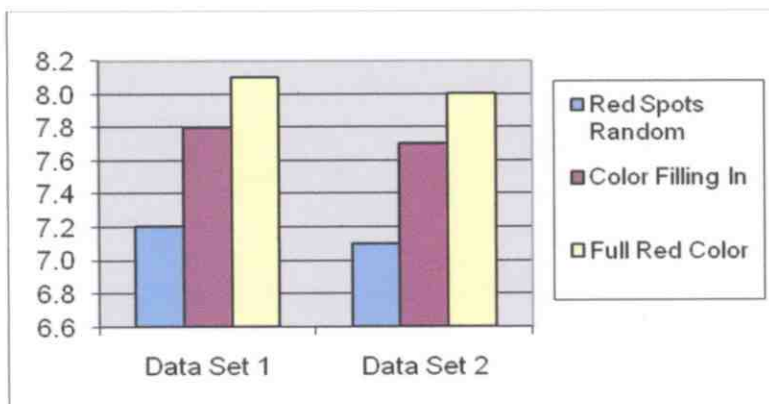

QUALITY ASSURANCE: APPROVED LOT #S8 100110

Edward N Sharpless
Laboratory Director

October 13, 2010
Date