

Safe-T-Vue® 6 • Product No. 7206

Quality Assurance: Safe-T-Vue® 6 Non-Reversible Blood Bag Temperature Indicator Product No. 7206

PLEASE NOTE: ALL BOX OF 50 INFORMATION AND FOIL LID COPY FOR SAFE-T-VUE® 6 IS PRINTED IN PURPLE.

Test performed on Random Sampling of Finished Product Lot # S6 042209

Expiration Date: April 2011

Non - Chemistry

Mark for "Accepted" and X for "Not Accepted."

Box	Adh. Label	Foil Lid	Close Function	Fill Level
Copy	Copy	Copy	Formed	Acceptable
Tack	Tack	Position	Locked/Stable	Underfill
Clean	Color	Clean Peel	Hinge	Overfill
Box Damage	Tray	Disk	Elasticity	Color Label
	Edges	Appearance		Color
	Color	Fit		

Test Protocol - Finished Goods Quality Assurance

Test performed on random sampling of finished product per ANSI ASQZ1.4-2003

Performed by using a "DigiSense" Thermister Electronic Thermometer. Using a cold (1° to 3° C) bag of simulated blood (a glycerol-water-red dye solution) with the electronic thermometer placed and sealed into the core of the blood bag to permit observation of temperature changes. Agitation of blood bag is necessary in the collection of accurate temperature-color data during receiving inspection. For detailed protocol, request QCP/0200-3 REV 01 07/07/07 - Receiving Inspection - Temperature Indicators. [Incoming inspection of 7206 has a specific incoming inspection protocol.]

Temperature Change and Corresponding Safe-T-Vue® Change

Sample Set 1	DATA	Sample Set 2
1 to 3 °C	<i>Starting Temperatures</i>	1 to 3 °C

OBSERVATIONS


Temperature	Condition
5.0 °C	Red Spots - WHITE CENTER Random
5.8 °C	Red Filling In WHITE CENTER
6.1 °C	Full Red Color RED CENTER

Temperature	Condition
5.0 °C	Red Spots - WHITE CENTER Random
5.7 °C	Red Filling In WHITE CENTER
6.1 °C	Full Red Color RED CENTER

Temperature accuracy is +/-0.3°C.

Results of Testing Lot # S6 042209; Test Date: May 14, 2009

Red Spots - Random 5.0 °C; Red Filling in White Center 5.8 °C; Full Red Color at 6.1 °C. **EXAMPLE GRAPH ONLY**

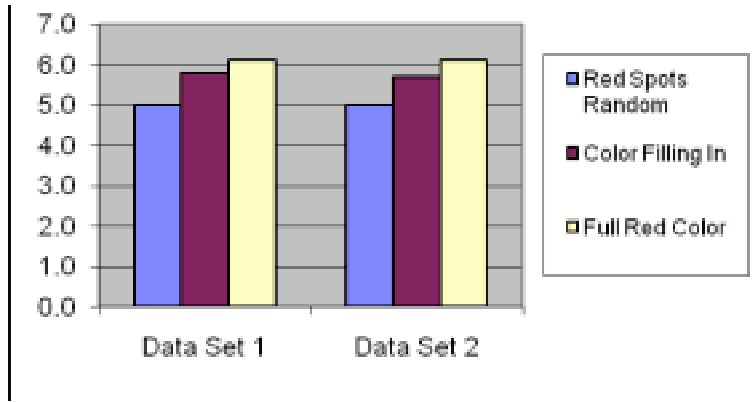

QUALITY ASSURANCE: APPROVED LOT # S6 042209 ; *Edward N. Sharpless*
QAP/0100-3 REV 02, July 8, 2007 Quality Director

May 14, 2009
Date