

**Safe-T-Vue® 10 • Product No. 7201**

**Quality Assurance: Safe-T-Vue® 10 Non-Reversible Blood Bag Temperature Indicator Product No. 7201**  
 PLEASE NOTE: ALL BOX OF 50 INFORMATION AND FOIL LID COPY FOR SAFE-T-VUE® 10 IS PRINTED IN BLACK.

Lot # **S10 051211**  
 Expiration Date: **2013-05**

**Non - Chemistry**

Mark ✓ for "Accepted" and X for "Not Accepted."

Box	Adh. Label	Foil Lid	Close Function	Fill Level
✓ Copy	✓ Copy	✓ Copy	✓ Formed	✓ Acceptable
✓ Tack	✓ Tack	✓ Position	✓ Locked/Stable	Underfill
✓ Clean	✓ Color	✓ Clean Peel	<b>Hinge</b>	Overfill
✓ Box Damage	<b>Tray</b>	<b>Disk</b>	✓ Elasticity	<b>Color Label</b>
	✓ Edges	✓ Appearance		✓ Color
	✓ Color	✓ Fit		

**Test Protocol – Finished Goods Quality Assurance**

*Test performed on random sampling of finished product per ANSI ASQZ1.4-2003*

Data collected using an electronic thermometer, 1° to 4° C start temperature, with Safe-T-Vue on a bag of simulated blood (10% glycerol-water), and thermister probe positioned in center of blood bag. Agitation of blood bag necessary for collection of accurate temperature-color change data. Download detailed SOP protocol in MS WORD, from [www.williamlabs.com](http://www.williamlabs.com), QAP/0102 REV 03 " Validation Procedure for Safe-T-Vue 10 (Product 7201) and Safe-T-Vue 8 (Product 7208)".

**Temperature Change and Corresponding Safe-T-Vue® Change**

Sample Set 1	DATA	Sample Set 2
1 to 4 °C	<i>Starting Temperatures</i>	1 to 4 °C


**OBSERVATIONS**

Temperature	Condition	
9.0 °C	Red Spots - Random	WHITE CENTER
9.7 °C	Red Filling In	WHITE CENTER
10.1 °C	Full Red Color	RED CENTER

Temperature	Condition	
9.0 °C	Red Spots – Random	WHITE CENTER
9.6 °C	Red Filling In	WHITE CENTER
10.1 °C	Full Red Color	RED CENTER

Temperature accuracy is +/-0.3°C.

**Results of Testing:** Red Spots - Random 9.0°C; Red Filling in White Center 9.7°C; Full Red Color at 10.1°C.

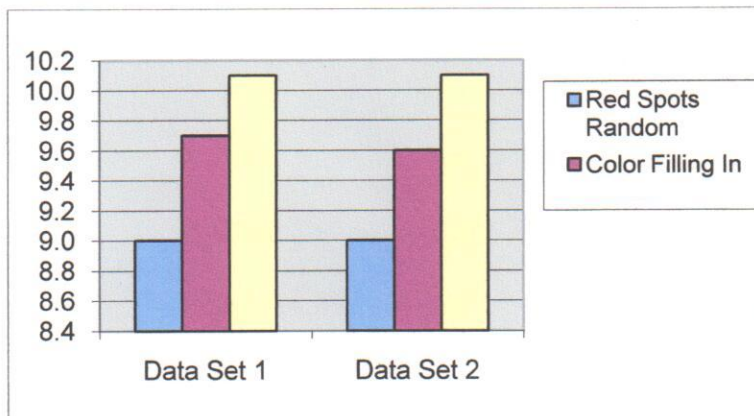

**QUALITY ASSURANCE: APPROVED LOT # S10 051211 ;** Edward N. Sharpless **July 13, 2011**  
 Laboratory Director Date